

상세규격서

구분	품명	단위	수량	비고
1	Ø1" Broadband Dielectric Mirror 400 - 750 nm 10 Pack	ea	6	
2	Ø2" Broadband Dielectric Mirror, 400 - 750 nm, 10 Pack	ea	6	


상세내역

1. 구성


1. Ø1" Broadband Dielectric Mirror 400 - 750 nm 10 Pack
2. Ø2" Broadband Dielectric Mirror, 400 - 750 nm, 10 Pack

2. 규격

1. Ø1" Broadband Dielectric Mirror 400 - 750 nm 10 Pack
 - Round Mirror Diameters: 1"
 - Broadband Coating Options : 400 - 750 nm
 - Fused Silica Substrates
 - $R_{avg} > 99\%$ for S- and P- Polarization for Angles of Incidence from 0 to 45°
 - Designed for CW and Nanosecond Lasers

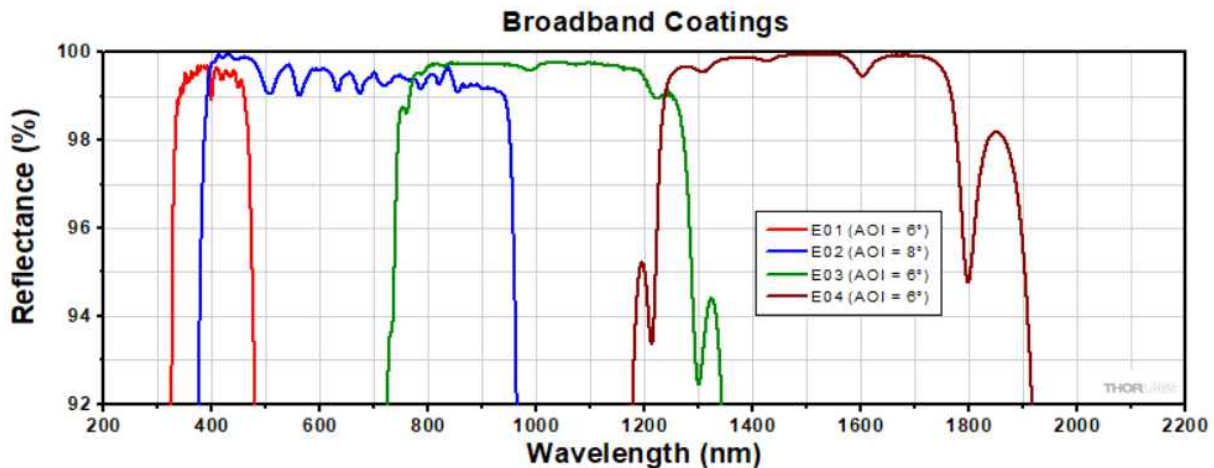

2. Ø2" Broadband Dielectric Mirror, 400 - 750 nm, 10 Pack
 - Round Mirror Diameters: 1"
 - Broadband Coating Options : 400 - 750 nm
 - Fused Silica Substrates
 - $R_{avg} > 99\%$ for S- and P- Polarization for Angles of Incidence from 0 to 45°
 - Designed for CW and Nanosecond Lasers



3. 기타사항

가. 설치위치 : 경북 구미시 구미대로 350-27 XR 디바이스 개발 지원센터 106호

나. 설치개요 : 규격서의 조건에 맞는 광학 소자 납품

다. 납품기한 : 계약일로 부터 14일 이내

라. 계약의 이행

- 1) 본 규격서에 대한 주계약자(이하 “계약자” 라 한다)와 발주기관 간의 해석상 이견은 발주기관의 해석에 따라야 하며, 본 규격서에 특별히 명시되지 않은 사항은 정부계약법 등의 규정과 일반 관례에 따른다.
- 2) 발주기관은 계약내용 전부에 대한 권리를 행사할 수 있으며 계약자는 이에 대하여 전적으로 동의해야 한다.
- 3) 본 규격서에 명시된 모든 조항은 본 사업의 원활한 추진에 필요한 최소한의 사항만을 규정하였으므로 상세히 기술하지 않았거나 누락된 사항에 대해서도 정상운영 및 서비스에 문제가 발생되지 않도록 계약자는 사전 조치를 취하여야 한다.
- 4) 본 규격서에서 요구하는 성능 및 특성에 대해 계약자의 오인 또는 누락된 상태로 계약 체결되어, 계약 후 이를 보완하기 위한 설계 변경, 물품 등을 추가해야 할 경우 계약자 부담으로 시행한다.
- 5) 계약자는 공급하는 제품의 성능, 품질 등에 대한 최종적인 책임을 진다.

4. 기타조건

가. 납품기한 : 계약 후 14일 이내

다. 규격관련 문의사항 : 강필성 선임연구원 : 010-4261-0006